

APPROVED	O.G. FIG.	
BY	CLASS	SUBCLASS
DRAFTSMAN		

002720-86E00960

Fig.1.

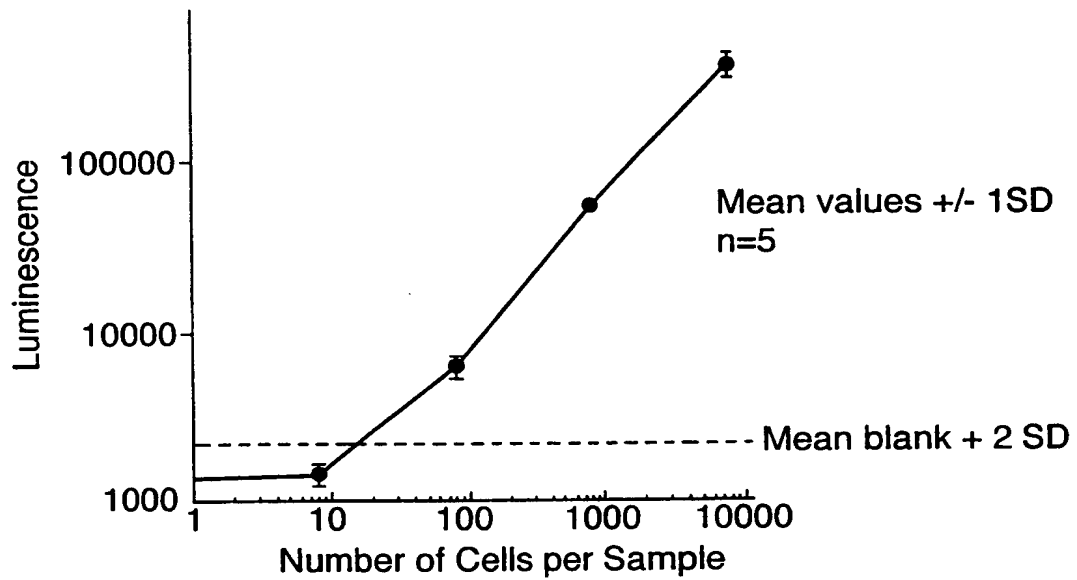


Fig.2.

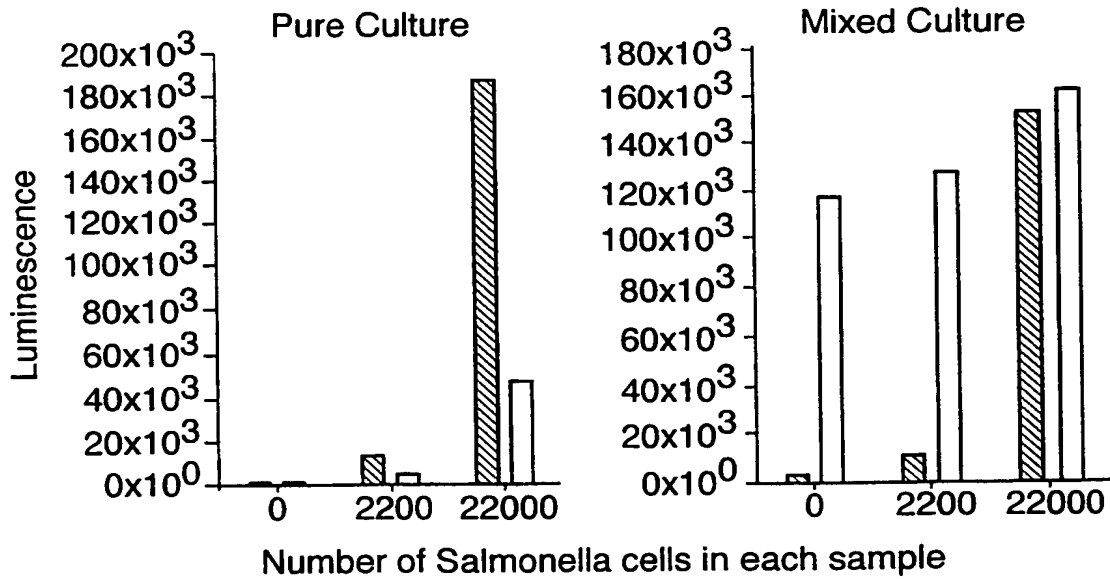


Fig.3.

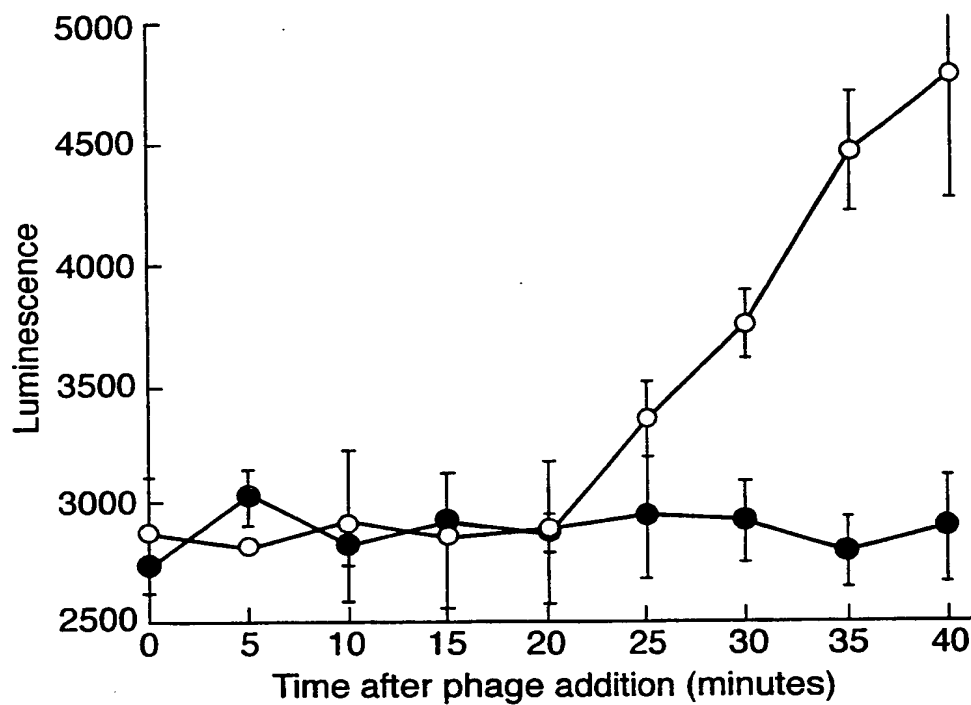


Fig.5.

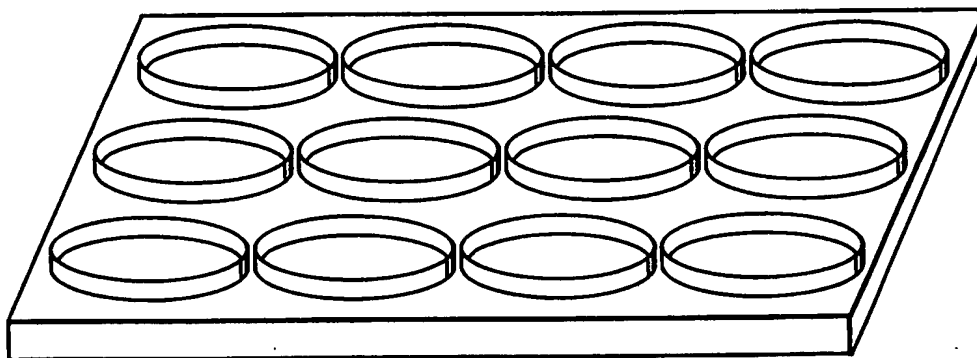



Fig.4.

Results from a test with a lytic antibiotic

No additions —	Plus antibiotic +	No additions —	Plus antibiotic —
Plus phage + +	Plus phage and antibiotic +	Plus phage + +	Plus phage and antibiotic + +
SUSCEPTIBLE		RESISTANT	

Results from a test with a non-lytic antibiotic

No additions —	Plus antibiotic —	No additions —	Plus antibiotic —
Plus phage + +	Plus phage and antibiotic —	Plus phage + +	Plus phage and antibiotic + +
SUSCEPTIBLE		RESISTANT	

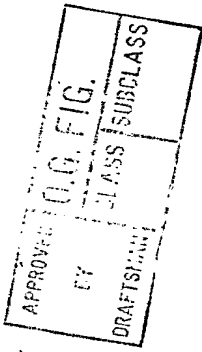

4/4

Fig.6.

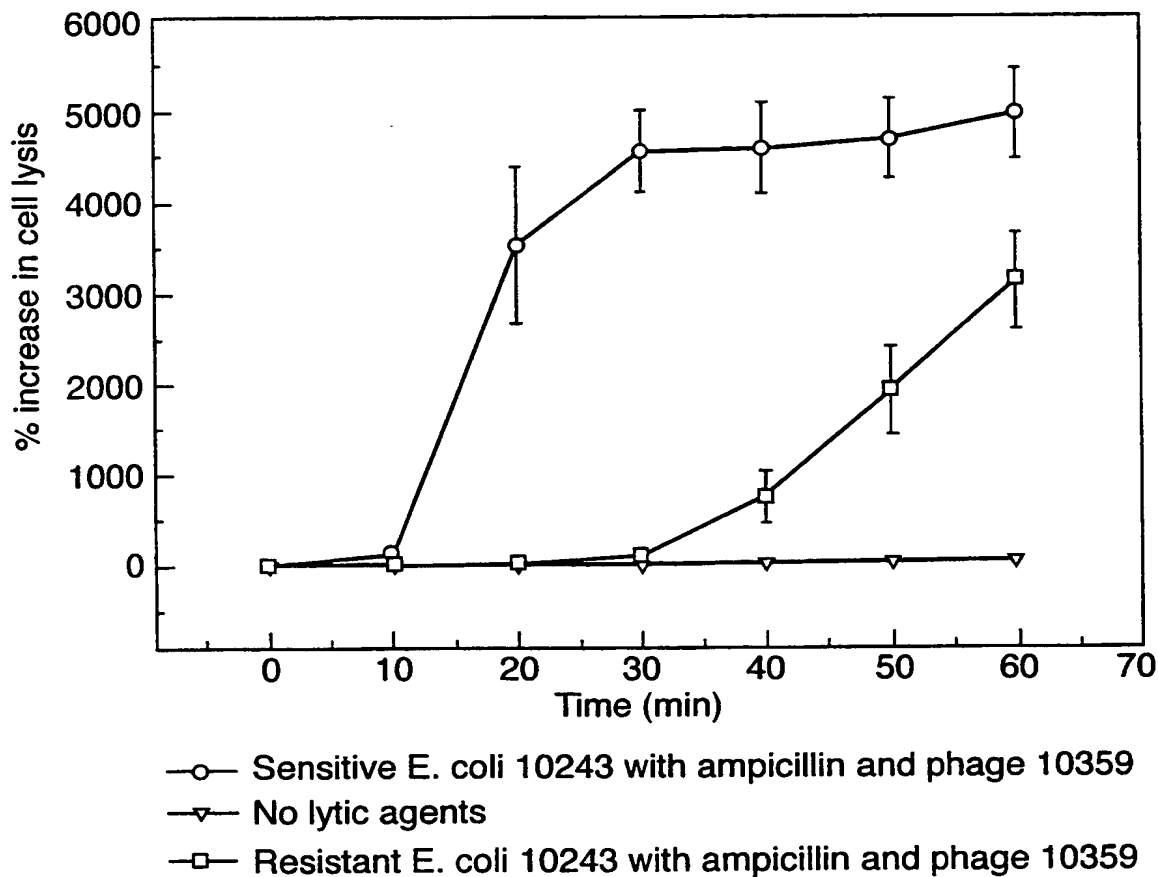


Fig.7.

